


# CLEANBRUSH® KIT-4, KIT-5

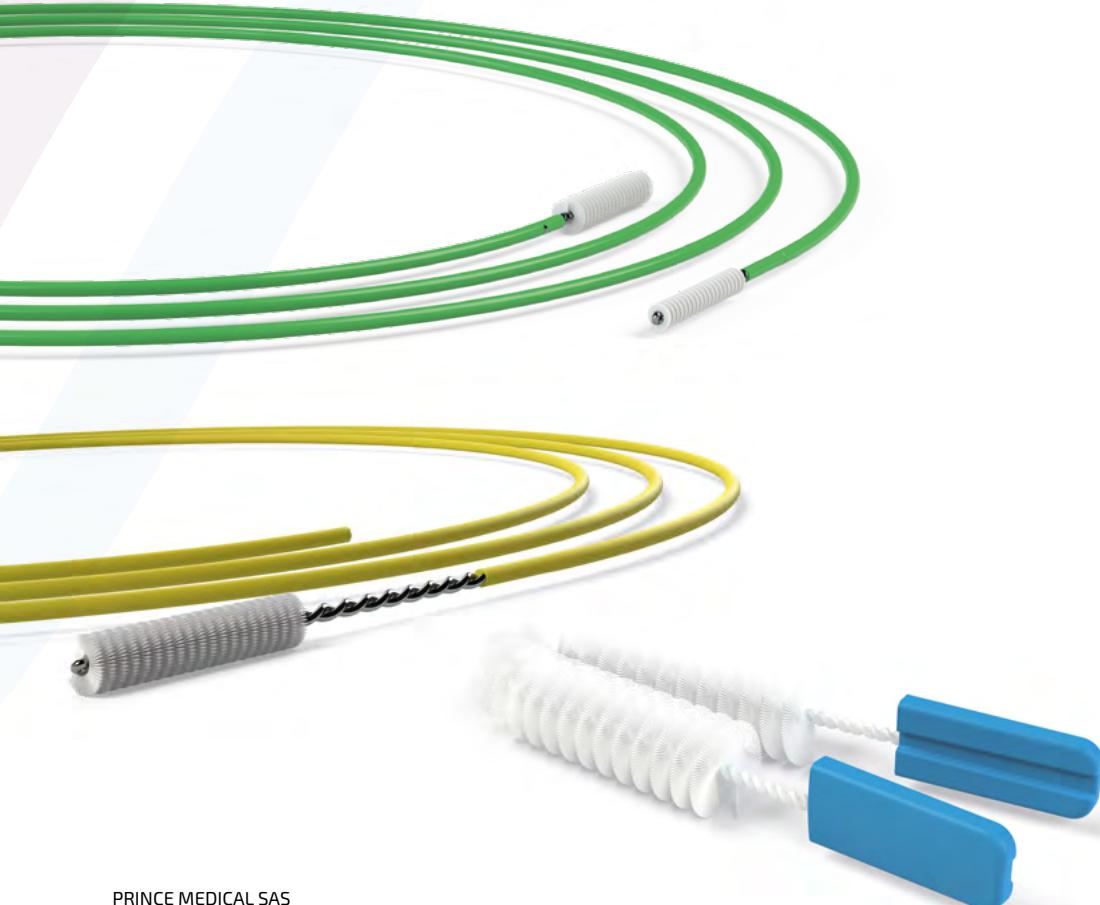

The CLEANBRUSH® KIT-4, KIT-5 swab kits are intended for cleaning the working channels, valves and valve cages of flexible endoscopes.

They are suitable for use with the main gastroscopes, colonoscopes, duodenoscopes, enteroscopes, bronchoscopes, cystoscopes, ureteroscopes, nephroscopes, hysteroscopes and naso-laryngoscopes on the market.

#### KIT COMPONENTS (SEE THE TABLE FOR THE DETAILED COMPONENTS BY REFERENCE)

- CLEANBRUSH® ENDO: cleaning brush for working channel
- CLEANBRUSH® ENDO (AN1055002, AN1055023, AN1056523): cleaning brush for the aspiration channel
- CLEANBRUSH® ENDO (AN1050123, AN1050138): cleaning brush for air/water channel, and/or Water Jet and/or balloon inflation channel
- CLEANBRUSH® PISTON: cleaning brush for valves, valve cages
- CLEANBRUSH® EXO-B: brush for external cleaning

#### ABOUT THIS MEDICAL DEVICE

1 <sup>st</sup> release date	1999
Single use	Yes
Class	I
Sterile	No (ethylene oxide decontamination)
Contains latex	No
Lifetime	5 years
Certification	CE
Packaging	Box of 25 or 50 units depending on product reference
Storage	In its original box in a cool and dry place

PRINCE MEDICAL SAS  
ZA La Sente Du Moulin  
64 rue Gutenberg - 60530 Ercuis - France  
[www.prince-medical.com](http://www.prince-medical.com)  
Tel: +33 (0)3 44 26 54 76  
[prince-medical@omerin.com](mailto:prince-medical@omerin.com)

**PRINCE MEDICAL**  
DEVICES

The information provided on this data sheet is indicative and subject to change without notice. PRINCE MEDICAL SAS shall not be held responsible for any incidents resulting from inappropriate use, failure to comply with the rules and regulations in force, or failure to follow the instructions for use provided. Medical devices sold by PRINCE MEDICAL SAS should only be used by a duly qualified practitioner or authorised person.

® Registered trademark of PRINCE MEDICAL SAS. Drawings and photos are not contractually binding. Reproduction is prohibited without the prior consent of PRINCE MEDICAL SAS.

## CLEANBRUSH® KIT-4, KIT-5

AVAILABLE  
REFERENCE(S)

&gt; KIT with 4 parts

Kit reference	REFERENCES FOR CLEANING BRUSHES					OTHER KIT COMPONENTS	65
	For working channel	For aspiration channel	For valves	For air/water channel, water jet, balloon inflation channel	External cleaning brush		
HN1903018	HN1053018 (with 1 brush Ø 3 mm L180 cm)	HN1055023 (with 1 brush Ø 5 mm L230 cm)					
HN1983018	HN1063018 (with 2 brushes Ø 3 mm L180 cm)	HN1056523 (with 1 brush Ø 6.5 mm L230 cm)		HN1050123 (with 1 brush Ø 1.8 mm L230 cm)			50
HN4535018	HN1065018 (with 2 brushes Ø 5 mm L180 cm)	HN1055002 (with 1 brush Ø 5 mm L20 cm)	HN106110 (with 2 brushes Ø 11 & 5 mm, L15.5 cm)				
HN2543010	HN1053010 (with 1 brush Ø 3 mm L100 cm)	HN1056523 (with 1 brush Ø 6.5 mm L230 cm)					
HN2553010	HN1063010 (with 2 brushes Ø 3 mm L100 cm)	HN1055002 (with 1 brush Ø 5 mm L20 cm)					
HN4505023	HN1055023 (with 1 brush Ø 5 mm L230 cm)	HN1056523 (with 1 brush Ø 6.5 mm L230 cm)					
HN4515023	HN1065023 (with 2 brushes Ø 5 mm L230 cm)						
HN4505018	HN1055018 (with 1 brush Ø 5 mm L180 cm)						
HN4515018	HN1065018 (with 2 brushes Ø 5 mm L180 cm)						
HN2543018	HN1053018 (with 1 brush Ø 3 mm L180 cm)			HN1050123 (with 1 brush Ø 1.8 mm L230 cm)			
HN2545023	HN1055023 (with 1 brush Ø 5 mm L230 cm)						
HN3335023	HN1065023 (with 2 brushes Ø 5 mm L230 cm)			HN1050138 (with 1 brush Ø 1.8 mm L380 cm)			
HN2995023	HN1055023 (with 1 brush Ø 5 mm L230 cm)						

AVAILABLE  
REFERENCE(S)  
> KIT with 5 parts

Kit reference	REFERENCES FOR CLEANING BRUSHES					OTHER KIT COMPONENTS	Packaging
	For working channel	For aspiration channel	For valves	For air/water channel, water jet, balloon inflation channel	External cleaning brush		
HN4545018	HN1055018 (with 1 brush Ø 5 mm L180 cm)	HN1056523 (with 1 brush Ø 6.5 mm L230 cm)	HN106110 (with 2 brushes Ø 11 & 5 mm, L15.5 cm)	HN1050123 (with 1 brush Ø 1.8 mm L230 cm)			
HN4555018	HN1065018 (with 2 brushes Ø 5 mm L180 cm)						25

The information provided on this data sheet is indicative and subject to change without notice. PRINCE MEDICAL SAS shall not be held responsible for any incidents resulting from inappropriate use, failure to comply with the rules and regulations in force, or failure to follow the instructions for use provided. Medical devices sold by PRINCE MEDICAL SAS should only be used by a duly qualified practitioner or authorised person.

\* Registered trademark of PRINCE MEDICAL SAS. Drawings and photos are not contractually binding. Reproduction is prohibited without the prior consent of PRINCE MEDICAL SAS.